Quanterix
The Science of Precision Health

Simoa™ IL-1alpha Discovery Kit
Certificate of Analysis

Product Number:	101968
Lot Number:	502351
Expiration:	22-Nov-2020
Platform(s):	HD-1/HD-X

Data below represents results generated on the Simoa™ HD-1 Analyzer.

Component	Part Number	Lot Number
Bead Stock	101966	002304
Detector Stock	101967	002109
Calibrator Concentrate	101965	000719
Calibrator Diluent	101963	932922
Sample Diluent	101964	932622

Generic Components - Included With Kit But Not Lot Number Specific	
Discovery Bead Diluent	101954
Discovery Detector Diluent	101955
Discovery SBG Diluent	101956
Discovery SBG Stock	103297
RGP Reagent	103159

Calibrator Concentrate Target Value	600 pg/mL

Calibration Curve

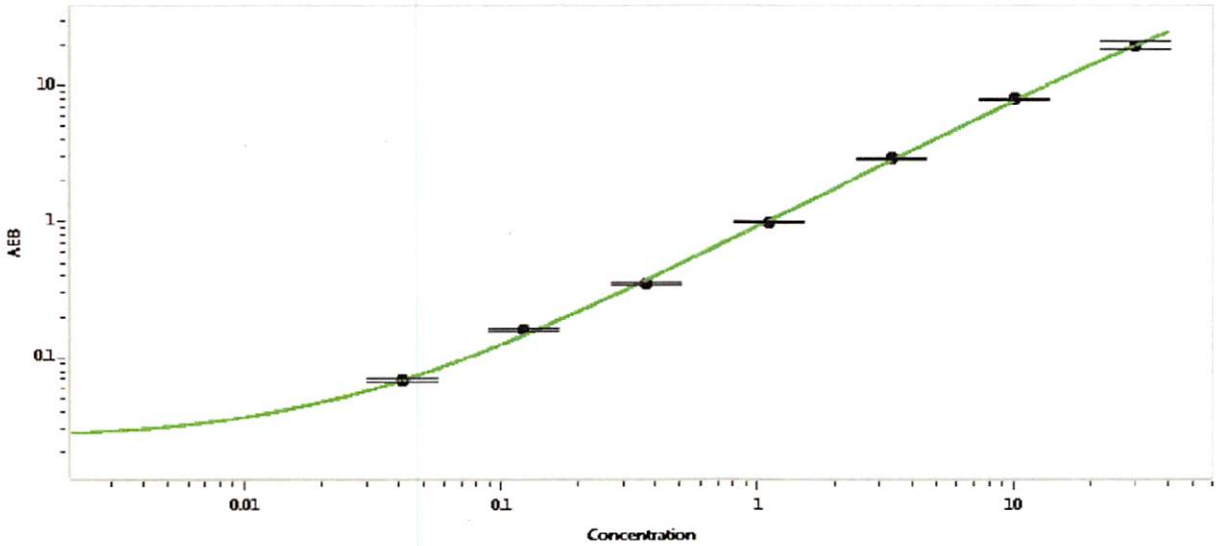

Calibrator Levels (pg/mL)	
A	0.000
B	0.041
C	0.123
D	0.370
E	1.11
F	3.33
G	10.0
H	30.0

Review/Approval	Name	Title	Signature/Date
	Shivam Goel	QC Manager	Shivam Goel 30Apr2020

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©2019 Quanterix, Inc. Simoa™ is a registered trademark of Quanterix, Inc
For research use only. Not for use in diagnostic procedures.