Quanterix
The Science of Precision Health

Simoa™ Tau 2.0 Kit
Certificate of Analysis

Product Number:	101552
Lot Number:	501982
Expiration:	13-Jun-2020
Platform(s):	HD-1/HD-x & SR-X

Data below represents results generated on the Simoa™ HD-1 Analyzer.

Component	Part Number	Lot Number
Bead Reagent	101554	922402
Detector Reagent	101553	921901
SBG Reagent	101555	921311
Sample Diluent	101556	921902
Calibrators	101559	922001
Controls	101560-101561	922002
SBG Diluent (SR-X)†	103158	N/A[1]
RGP Reagent	103159	N/A[1]

[1] RGP is not Kit Lot Specific

Release Materials*			
	Lot	Result (pg/mL)	Mean Range (pg/mL)
Control 1	922002	0.994	0.748-1.24
Control 2	922002	51.5	43.0-64.5
Panel 1	916901	1.27	0.640-1.55
Panel 2	916902	1.76	1.19-2.11
Panel 3	916903	23.1	17.2-29.5
Panel 4	916904	74.3	63.4-95.0

* Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibration Curve

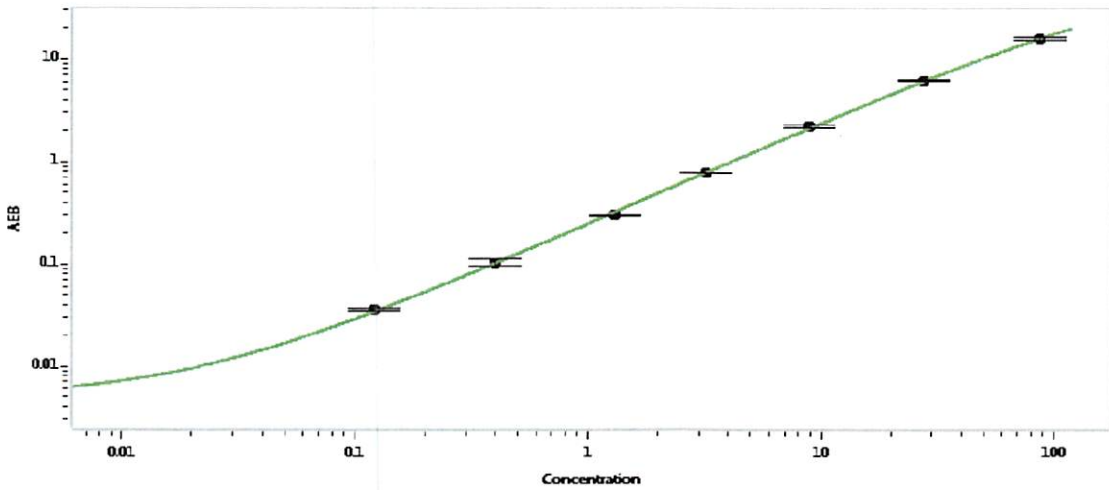

Calibrator Levels (pg/mL)	
A	0.000
B	0.121
C	0.399
D	1.30
E	3.21
F	8.83
G	27.4
H	87.5

Review/Approval	Daniel Ritchie	Senior QC Analyst	19 Aug 2019
	Name	Title	Signature/Date

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©2019 Quanterix, Inc. Simoa™ is a registered trademark of Quanterix, Inc
For research use only. Not for use in diagnostic procedures.