Quanterix
The Science of Precision Health

Simoa® NF-light Advantage Kit
Certificate of Analysis

Product Number:	103186
Lot Number:	503284
Expiration:	25-May-2022
Platform(s):	HD-1/ HD-X

Component	Part Number	Lot Number
Bead Reagent	102246	114511
Detector Reagent	102248	114512
SBG Reagent	102250	114513
Sample Diluent	102252	114514
Calibrators	102255	134704
Control 1	102256	134705
Control 2	102257	134705
RGP Reagent	103159	N/A[1]

[1] RGP is not Kit Lot Specific

Data below represents results generated on the Simoa HD-1® Analyzer.

Release Materials*			
	Lot	Result (pg/mL)	Mean Range (pg/mL)
Control 1	134705	3.53	3.20-4.80
Control 2	134705	257	224-336
Panel 1	134208	6.13	3.95-9.43
Panel 2	134208	3.84	1.86-7.15
Panel 3	134208	66.5	49.9-74.8
Panel 4	135805	365	274-411

* Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibration Curve

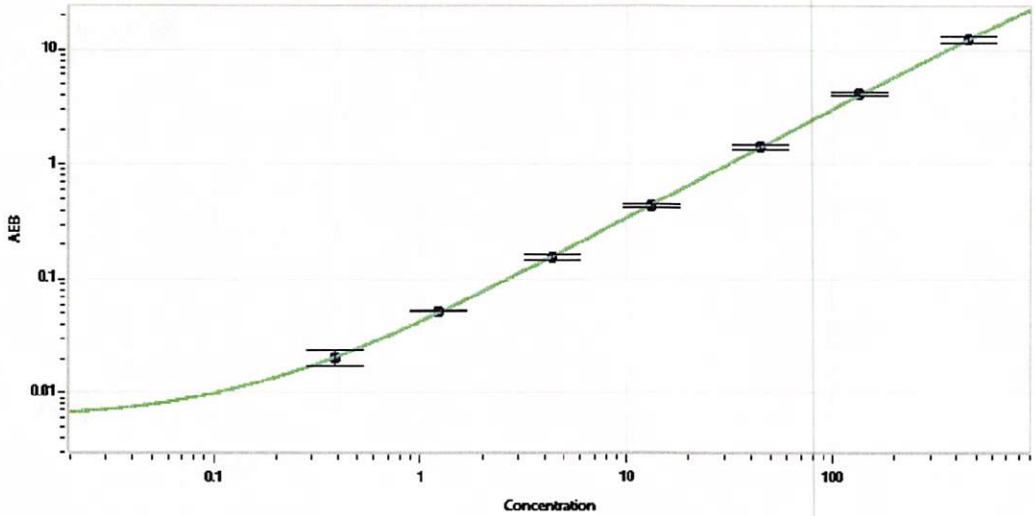

Calibrator Levels (pg/mL)	
A	0.000
B	0.391
C	1.22
D	4.35
E	13.2
F	44.8
G	134
H	456

Review/Approval	Name	Title	Signature/Date
	Shivani Goel	QC	Shivani Goel 12 Jan 2022

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©2019 Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures