Quanterix
The Science of Precision Health

Simoa® NF-Light SR-X Kit
Certificate of Analysis

Product Number:	103400
Lot Number:	503303
Expiration:	27-Aug-2022
Platform(s):	SR-X

Component	Part Number	Lot Number
Bead Reagent	102246	124505
Detector Reagent	102248	123907
SBG Reagent	102250	206707
Sample Diluent	103399	135010
Calibrators	102255	133605
Control 1	102256	133606
Control 2	102257	133606
RGP Reagent	103159	N/A[1]

[1] RGP Reagents are not Kit Lot Specific

Data below represents results generated on the Quanterix SR-X® Ultra-Sensitive Biomarker Detection System

Release Materials			
	Lot	Result (pg/mL)	Mean Range (pg/mL)
Control 1	133606	4.64	2.84 - 5.64
Control 2	133606	229	199 - 299
Panel 1	134208	6.69	3.95 - 9.43
Panel 2	134208	5.75	1.86 - 7.15
Panel 3	134208	63.7	49.9 - 74.8
Panel 4	135801	305	274 - 411

Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

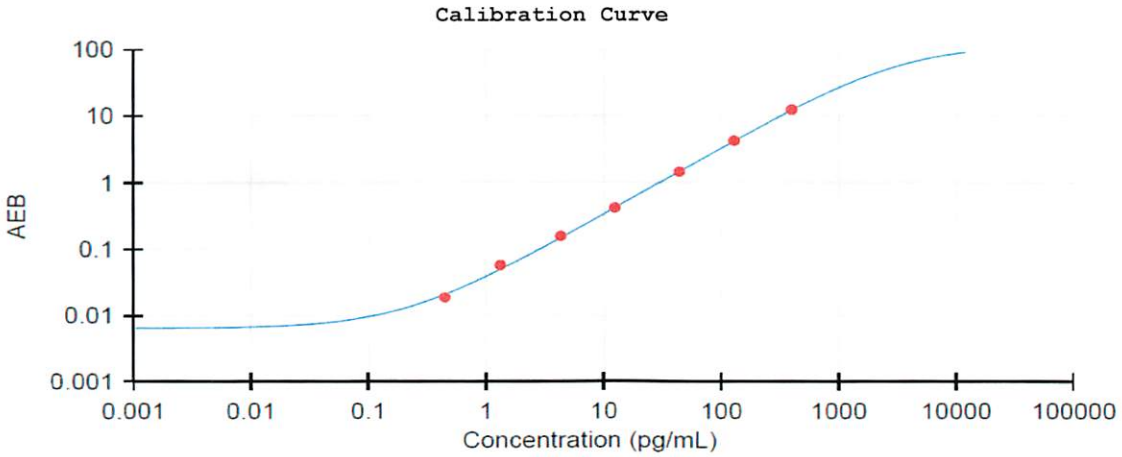

Calibrator Levels (pg/mL)	
A	0.000
B	0.447
C	1.33
D	4.33
E	12.5
F	44.2
G	129
H	400

Review/Approval	Shivani Goel	QC Manager	Shivani Goel 17 Mar 2022
	Name	Title	Signature/Date

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

© 2022 Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures