Quanterix
The Science of Precision Health

Simoa® IFNg 2.0 Kit
Certificate of Analysis

Product Number:	103337
Lot Number:	503365
Expiration:	15-Feb-2023
Platform(s):	HD-1/HD-X & SR-X

Component	Item Number	Lot Number
Bead Reagent	103334	205005
Detector Reagent	101091	205101
SBG Reagent	101101	205102
Sample Diluent	103336	205103
Calibrator Diluent	101095	204611
Calibrator Concentrate	101093	208601
RGP Reagent	103159	N/A[1]

[1] RGP is not Kit Lot Specific

Data below represents results generated on the Simoa® HD-1 / HD-X & SR-X Analyzer.

Release Materials*			
	Lot	Result (pg/mL)	Mean Range (pg/mL)
Control 1	206704	1.32	1.08-1.63
Control 2	206704	28.5	21.5-32.3
Panel 1	211906	1.64	1.29-2.22
Panel 2	211906	3.51	2.45-4.13
Panel 3	211906	33.4	22.4-39.8

* Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibrator Concentrate Value Assignment (pg/mL)	2,026

Calibration Curve

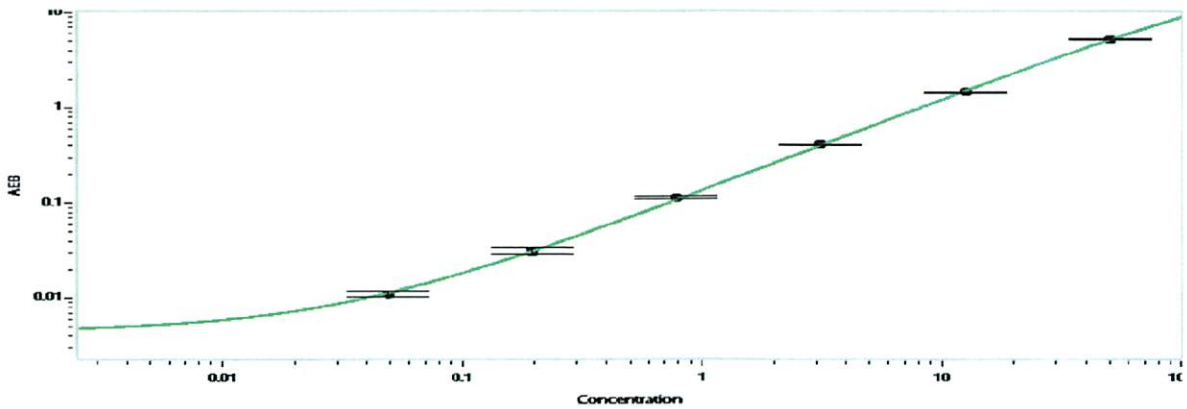

Calibrator Levels (pg/mL)	
A	0.000
B	0.049
C	0.195
D	0.781
E	3.13
F	12.5
G	50.0

Review/Approval

Name	Title	Signature/Date
Matt Smart	QC	20 May 2022

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures