Quanterix
The Science of Precision Health

Simoa® BDNF Discovery Kit
Certificate of Analysis

Product Number:	102039
Lot Number:	503658
Expiration:	23-May-2023
Platform(s):	HD-1/HD-X & SR-X

Component	Part Number	Lot Number
Bead Stock	102028	221601
Detector Stock	102029	222901
Calibrator Concentrate	102032	220716
Calibrator Diluent	102030	218617
Sample Diluent	103402	220715

Generic Components - Included With Kit But Not Lot Number Specific	
Discovery Bead Diluent	101954
Discovery Detector Diluent	101955
Discovery SBG Diluent	101956
Discovery SBG Stock	103297
RGP Reagent	103159

Data below represents results generated on the Simoa® HD-X Analyzer.

Calibrator Concentrate Target Value (ng/mL)	2.00

Calibration Curve

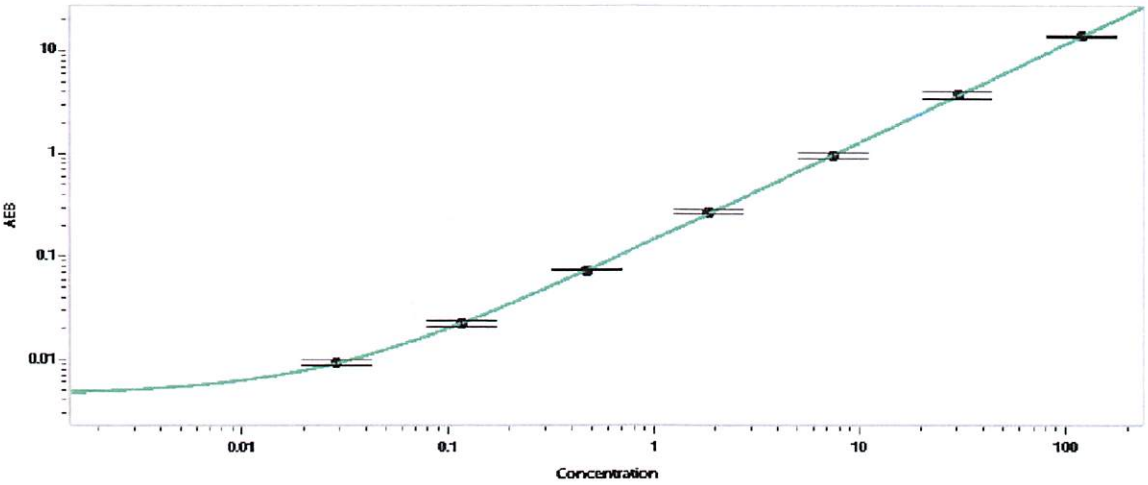

Calibrator Levels (pg/mL)	
A	0.000
B	0.029
C	0.117
D	0.469
E	1.88
F	7.50
G	30.0
H	120

Review/Approval

Name	Title	Signature/Date
Sonia Khillan	QC Manager	Sonia Khillan/24AUG2022

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnositic procedures