Quanterix
The Science of Precision Health

Simoa™ NF-Light SR-X Kit
Certificate of Analysis

Product Number:	103400
Lot Number:	503214
Expiration:	25-May-2022
Platform(s):	SR-X

Component	Part Number	Lot Number
Bead Reagent	102246	114511
Detector Reagent	102248	114512
SBG Reagent	102250	114513
Sample Diluent	103399	115909
Calibrators	102255	130504
Control 1	102256	130505
Control 2	102257	130505
RGP Reagent	103159	N/A[1]

[1] Reagents are not Kit Lot Specific

Data below represents results generated on the Quanterix SR-X™ Ultra-Sensitive

Release Materials			
	Lot	Result (pg/mL)	Mean Range (pg/mL)
Control 1	130505	4.24	2.99-4.57
Control 2	130505	154	111-225
Panel 1	008501	12.0	8.59-20.5
Panel 2	008501	8.69	7.39-15.1
Panel 3	008501	60.3	43.8-91.8
Panel 4	009401	203	128-302

Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibration Curve

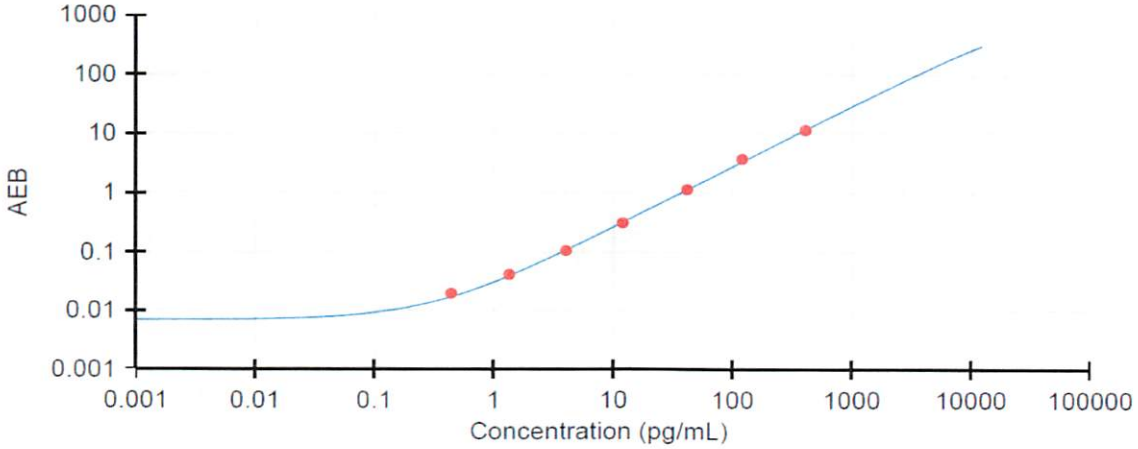

Calibrator	Levels (pg/mL)
A	0.000
B	0.439
C	1.35
D	4.02
E	12.0
F	41.6
G	120
H	407

Review/Approval — Matt Smart (Name) — Director, QC (Title) — [signature] 17Jun2022 (Signature/Date)

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©2019 Quanterix, Inc. Simoa™ is a registered trademark of Quanterix, Inc
For research use only. Not for use in diagnostic procedures.