Quanterix
The Science of Precision Health

Simoa® IL-6 2.0 Kit
Certificate of Analysis

Product Number:	101622
Lot Number:	503938
Expiration:	14-Aug-2024
Platform(s):	HD-1 / HD-X & SR-X

Component	Part Number	Lot Number
Bead Reagent	104233	324408
Detector Reagent	104347	325101
SBG Reagent	104349	325004
Sample Diluent	104351	323617
Calibrator Diluent	101627	322623
Calibrator Concentrate	100652	325803
RGP Reagent	103159	N/A[1]

[1] RGP is not Kit Lot Specific

Data below represents results generated on the Simoa® HD-1 / HD-X & SR-X Analyzer.

Release Materials*			
	Lot	Result (pg/mL)	Spec. Range (pg/mL)
Control 1	108406	1.56	1.23-1.92
Control 2	108406	21.7	17.5-28.9
Panel 1	029301	55.8	39.8-59.7
Panel 2	029401	6.17	4.35-6.53
Panel 3	029301	1.50	1.22-1.82

* Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibrator Concentrate Value Assignment (pg/mL)	492

Calibration Curve

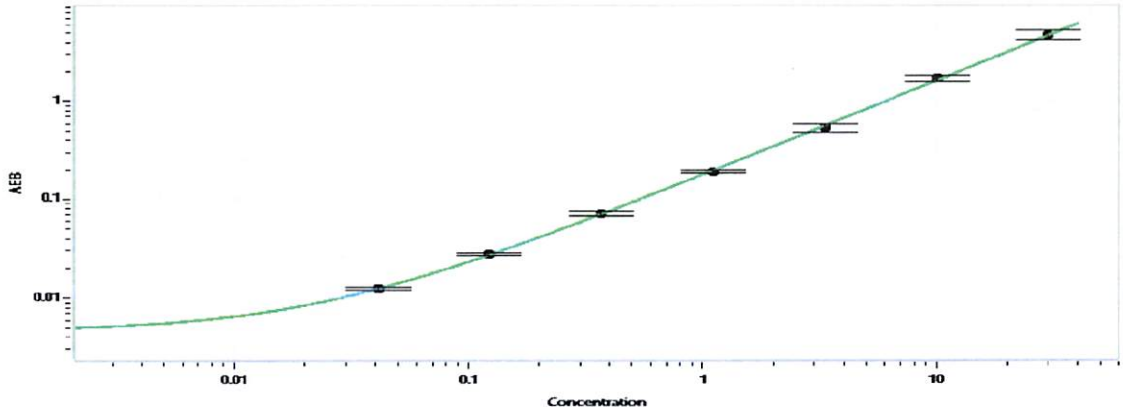

Calibrator Levels (pg/mL)	
A	0.00
B	0.041
C	0.123
D	0.370
E	1.11
F	3.33
G	10.0
H	30.0

Review/Approval

Name	Title	Signature/Date
ROBERT SOMOGYI	QC, MANAGOR	28SEP 2023

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnositic procedures