Quanterix®

Discovery Fueled by Ultra-Sensitivity

Simoa® NF-Light v2 Advantage Kit

Certificate of Analysis

Product Number:	104073
Lot Number:	504327
Expiration Date:	9-Jan-26
Platform(s):	SR-X and HD-1/HD-X

Component	Part Number	Lot Number
Bead Reagent	104067	421101
Detector Reagent	104068	421102
SBG Reagent	104069	421103
Sample Diluent Reagent	104071	421104
Reference Calibrators	102255	420801
Control 1	102256	420802
Control 2	102257	420802
RGP Reagent	103159	N/A[1]

[1] Reagents are not Kit Lot Specific

Data below represents results generated on the Simoa® HD-X Analyzer.

Release Materials*

NF-Light®

	Lot	Result (pg/mL)	Spec. Range (pg/mL)
Control 1	420802	3.91	3.01 - 4.95
Control 2	420802	225	182 - 273

*** Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.**

Calibration Curve

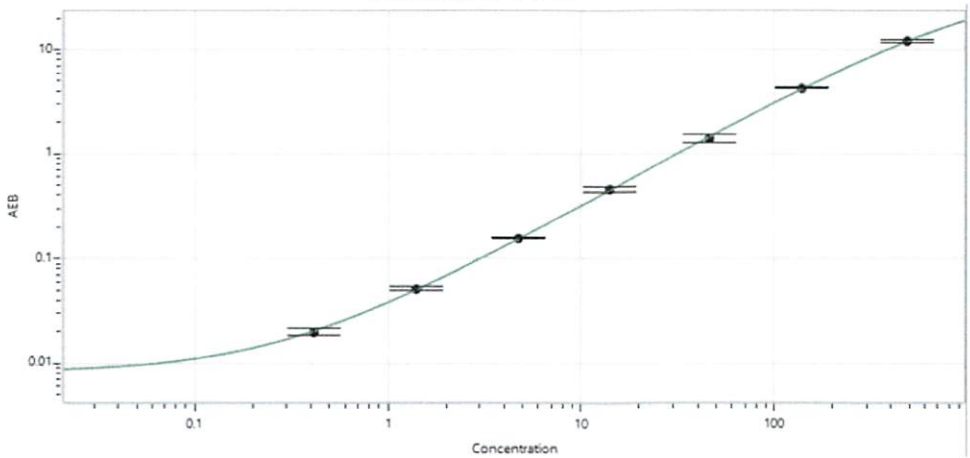

Calibrator Levels (pg/mL)	
A	0.000
B	0.417
C	1.41
D	4.74
E	14.1
F	46.2
G	139
H	487

Review/Approval Dipesh Patel Doc control-2 QA 30Aug2024

Name Title Signature/Date

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, 01821
techsupport@quanterix.com

©2024 Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures.

COA-0049 02